ROCAMED

JFIL®

New Ureteral Stent Generation with No Bladder Loop

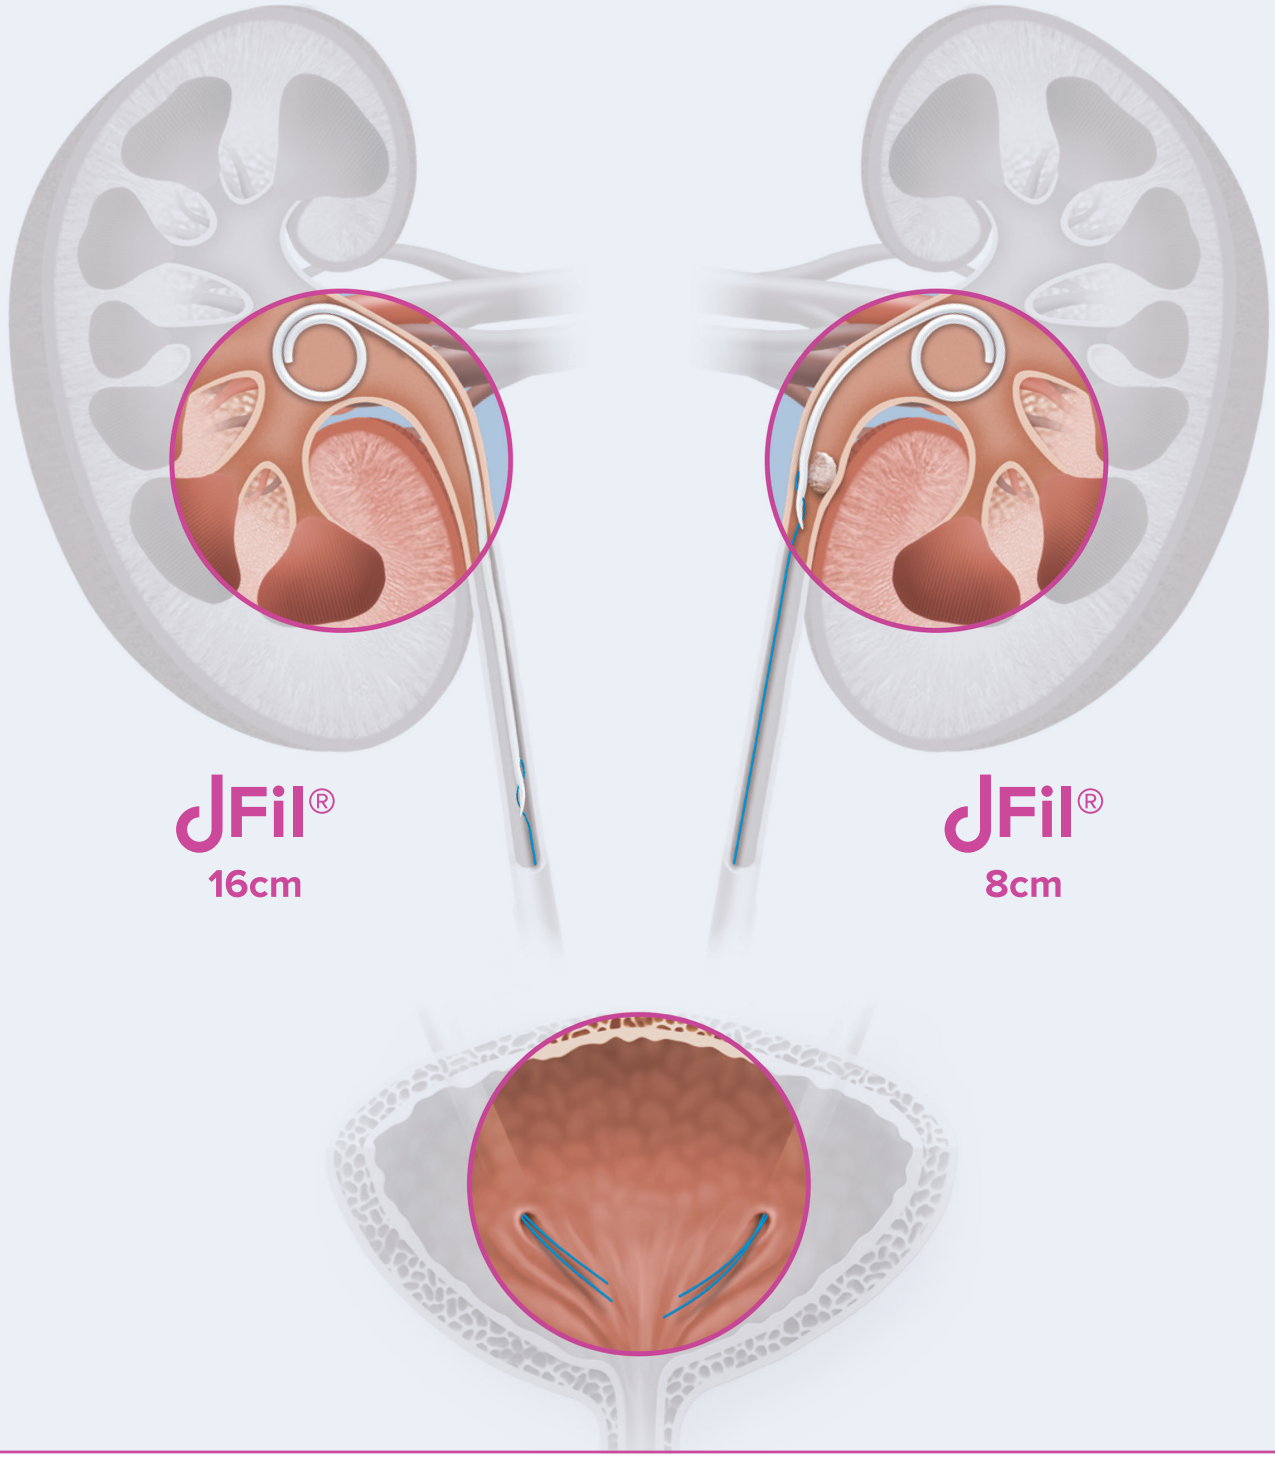

edap tms
Bringing New Horizons to Therapy

エダップテクノメド株式会社

JFil®

New Ureteral Stent Generation with No Bladder Loop

ROCAMED

Indications:

	Indwelling Time	Pre Operatory Dilatation	UPJ Obstructive Stone	Non Obstructive Stone
JFil®	Up to 30 days	✓	✓	✓

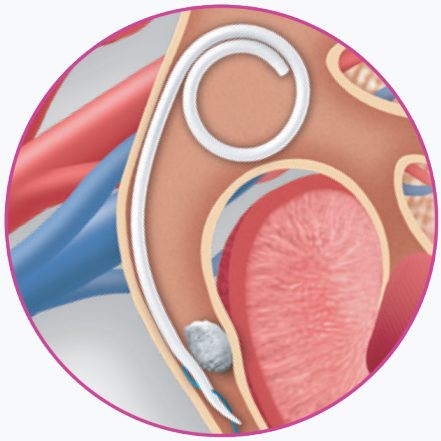

» Smooth dilation of the ureter by sutures

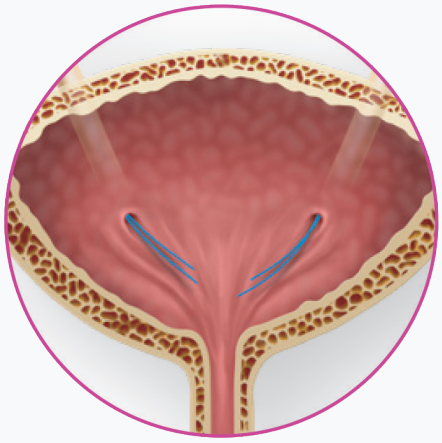

Literature:

Changing the double pigtail stent by a new suture stent to improve patient quality of life: A prospective study.
B. Vogt et al. World Journal of Urology 2015, 33(8):1061-8.

MiniJFil®: A new safe and effective stent for a well-tolerated repeated extracorporeal shockwave lithotripsy or ureteroscopy for medium-to-large kidney stones?
B. Vogt et al. Nephro-Urology Monthly 2016, 13;8(5):e40788.

Advances in ureteral stent development.
B.H. Chew et al. Current Opinion in Urology 2016, 26(3):277-82.

Prevention and treatment of symptoms associated with indwelling ureteral stents: A systematic review.
P. Betschart et al. International Journal of Urology 2017, 24(4):250-9.

Ureteral stents in urolithiasis.
M. Beysens et al. Asian Journal of Urology 2018, 5(4):274-86.

製品情報

商品コード	商品名	①ステント：Jfilステント		②ガイドワイヤ：Rocawireニチノール	
		JAN	JMDN	JAN	JMDN
ROJV0708ST	JFil 尿管スーチャーステントセット 7Fr 8cm	4582323373277	34926022 短期使用尿管用チューブステント	4582323373314	35094022 非血管用ガイドワイヤ
ROJV0716ST	JFil 尿管スーチャーステントセット 7Fr 16cm	4582323373284			

●包装単位：1セット / 1箱
セット構成：尿管スーチャーステント・メタルリング付きコネクタブルプッシャー・親水性ニチノールガイドワイヤ 150cm 0.035inch
① 販売名：Jfilステント　製造販売認証番号：304ADBZX00031000　クラス分類：Ⅱ
② 販売名：Rocawireニチノール　製造販売認証番号：301AFBZX00055000　クラス分類：Ⅱ

製造販売元：エダップテクノメド株式会社　www.edaptechnomed.co.jp

東京本社　〒104-0033 東京都中央区新川1-3-17　Tel 03-5540-6767　Fax 03-5540-6785
大阪営業所　〒532-0011 大阪市淀川区西中島5-3-10　Tel 06-6304-0960　Fax 06-6304-0876
福岡営業所　〒816-0912 福岡県大野城市御笠川5-3-4　Tel 092-600-7155　Fax 092-600-7166

本カタログに掲載した製品の仕様、外観は予告なく変更することがあります。

BFE202112